


VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program


JUL 29 2010

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130287 ✓
Name	Mitchell LANGSETH	ID#	2612 ✓
		Date	7/28/10 ✓
A	Agency	KENAI PD	Phone # 907-283-7827
	Instrument Location	Wildwood Pretrial	
B	Alco S/N	75509 ✓	Target Value .077 ✓
		High Pressure	250
	Alco Test Values	.077 ✓ 1st Alco	.076 ✓ 2nd Alco
	Signature		
		COB 7/30/10	
(OVER)			


(Do Not write in the area below)

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:



- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

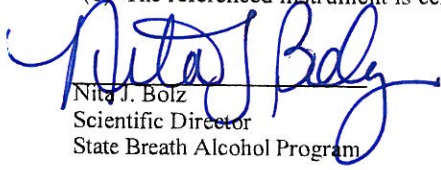
Nita J. Bolz
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 9th day of AUGUST, 2010.


Daniel L. Nicholas
Notary Public, State of Alaska
Commission Expires with Office

(Notary Seal Stamp)

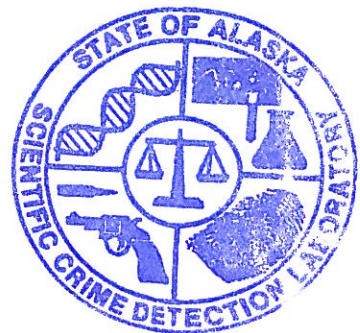

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N

130287

7/29/10
643

(CONTINUED FROM FRONT PAGE)

C

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130287

JULY 28, 2010

OPERATOR'S NAME:

LANGSETH

OPERATOR'S NUMBER: 2612

SUBJECT'S LAST NAME:

VERIFICATION OF CAL

SUBJECT'S FIRST NAME/MI :

U

O.L. #: 0

DEPT/AGENCY: KEN1

CASE/REPORT: 0

TEST TYPE: U

ALCO TARGET VALUE: .077

ALCO S/N: 75509

--- BREATH ANALYSIS ---

.077 ADJUSTED FOR 30.09 in
ALCO TARGET .077 01:50
BLANK TEST .000 01:51
INTERNAL STANDARD VERIFIED 01:51
ALCO TU 30.09 in .077 01:52
BLANK TEST .000 01:52
SUBJECT SAMPLE .000 01:53
BLANK TEST .000 01:54
ALCO TU 30.09 in .076 01:54
BLANK TEST .000 01:55

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130287

JULY 28, 2010

TIME 01:48

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 02/20/01

HEATERS

SAMPLE CHAMBER: 48c

BREATH TUBE: 41c

BAROMETER: 30.09 in

FLOW DETECTOR: OKAY

PUMP

HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

! " # \$ % ' () * + , - . / 0 1 2 3 4 5 6 7 8 9 : ; < = > ? @ A B C D E F G
H I J K L M N O P Q R S T U V W X Y Z [\] ^ _ ` a b c d e f g h i j k l m n o
p q r s t u v w x y z { | } ~ ¡ ¢